

FIG. 1

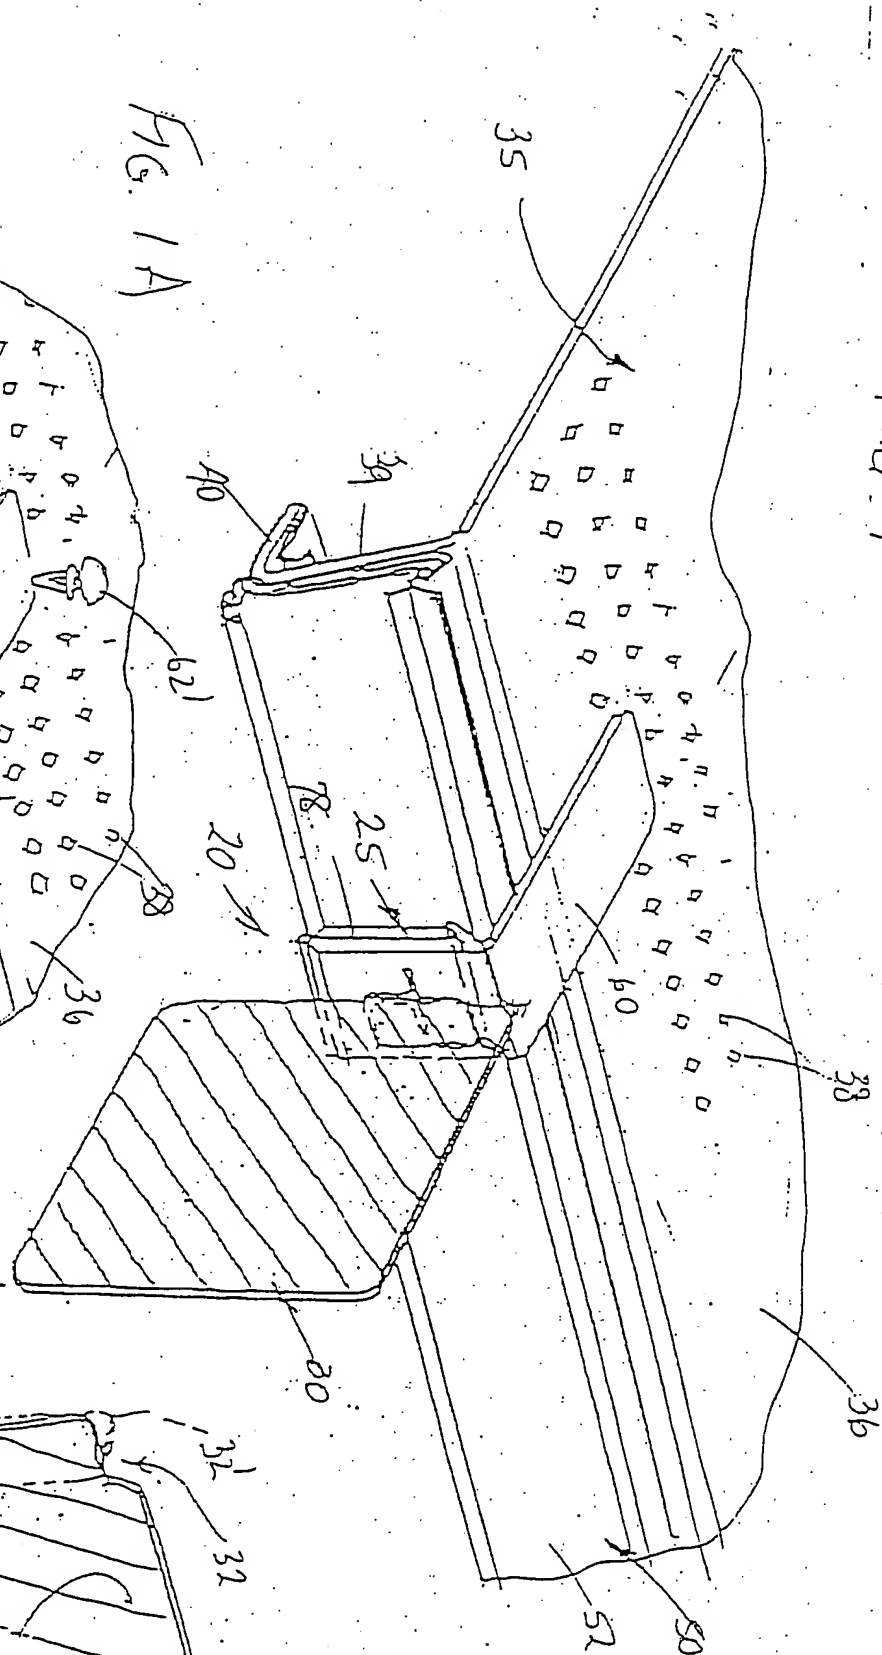


FIG. 1A

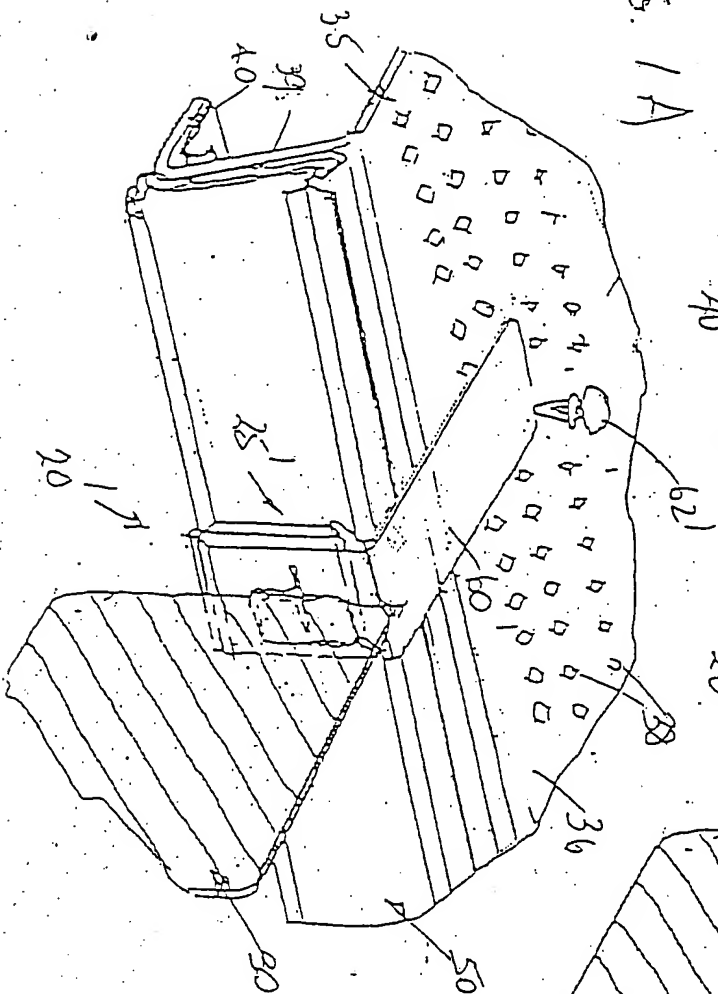
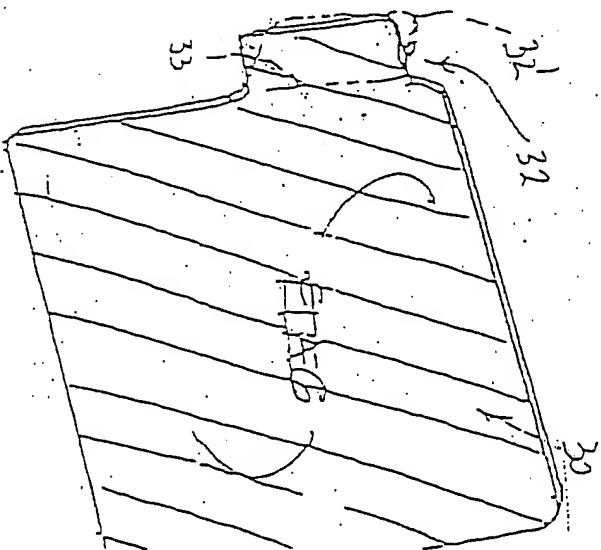


FIG. 5



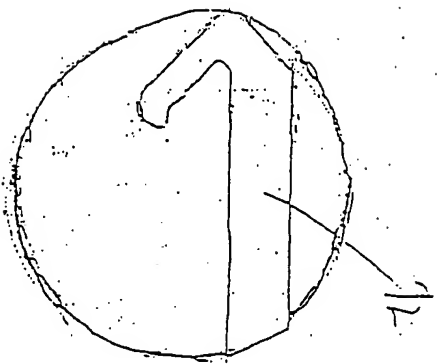


FIG. 5

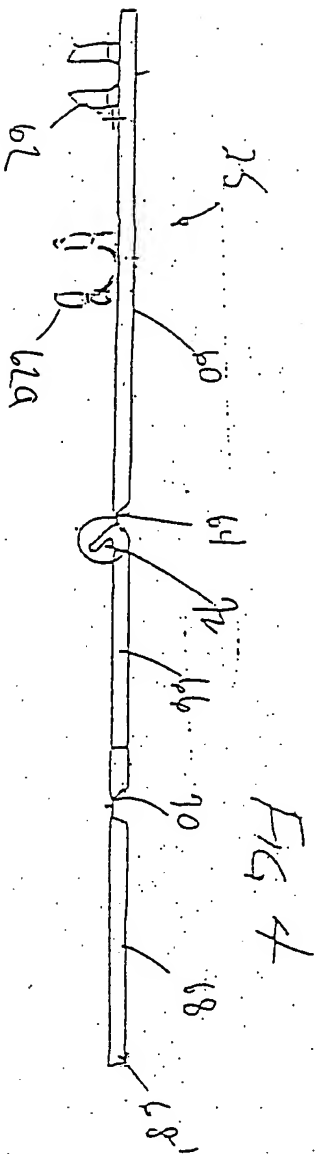


FIG. 4

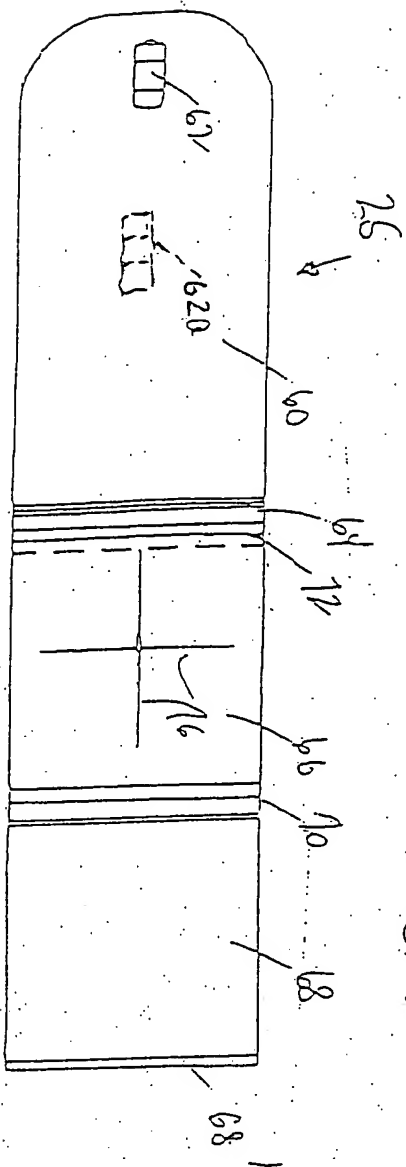


FIG. 3

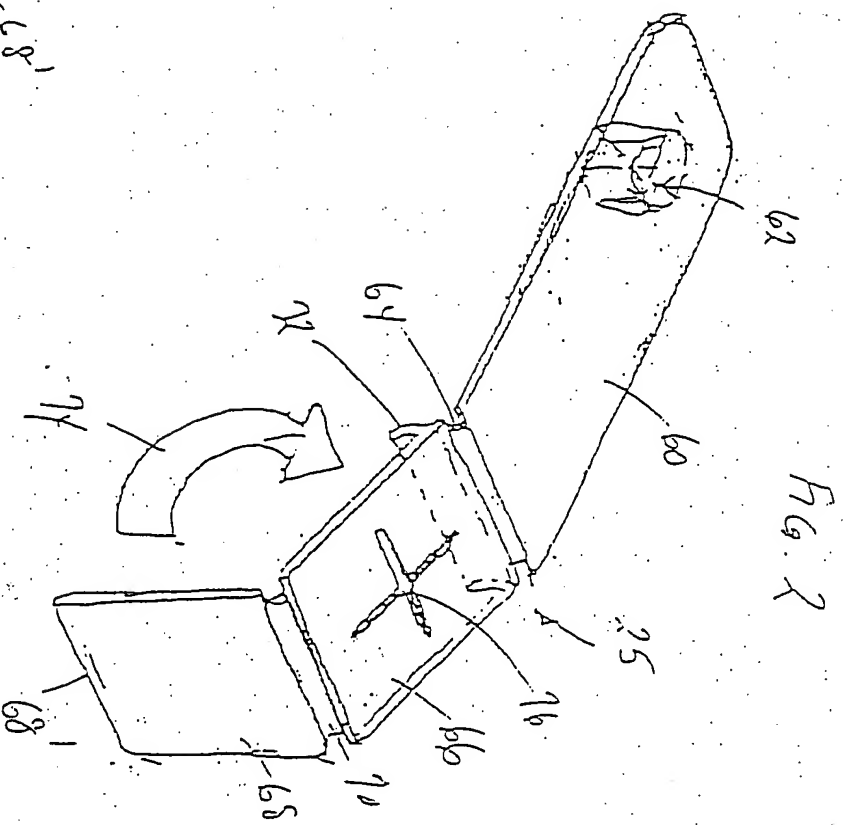


FIG. 2

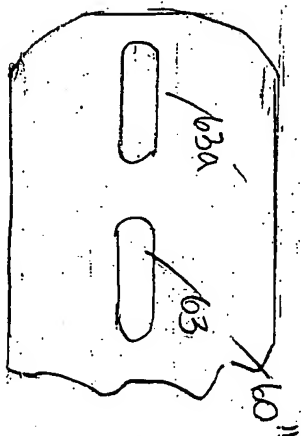


FIG. 3B

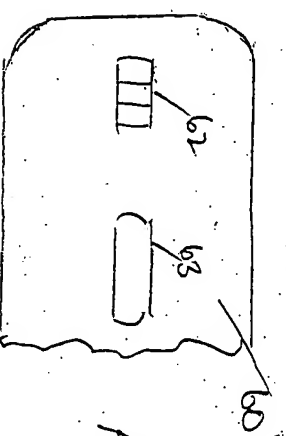


FIG. 3A

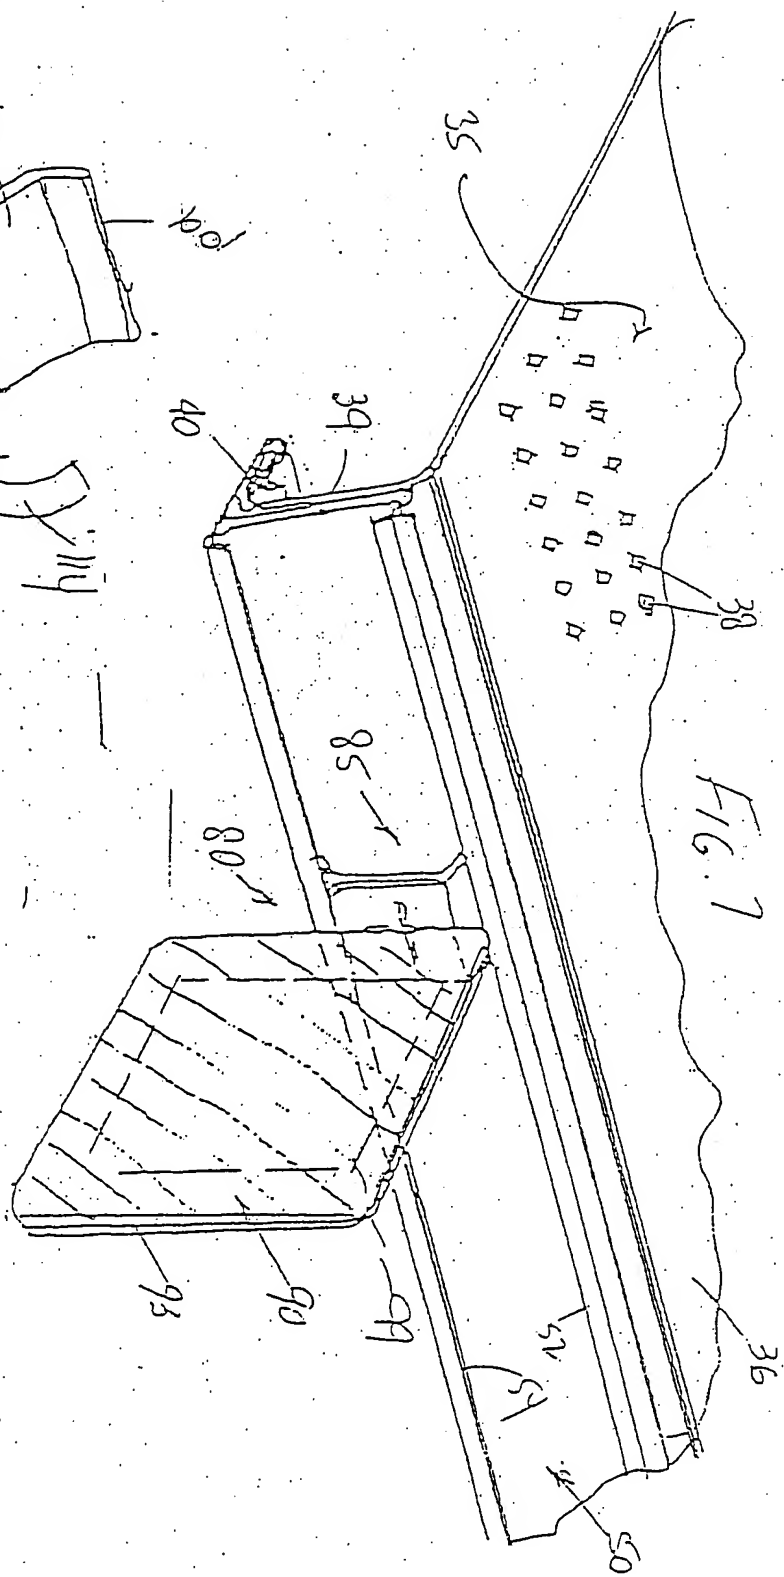


FIG. 7






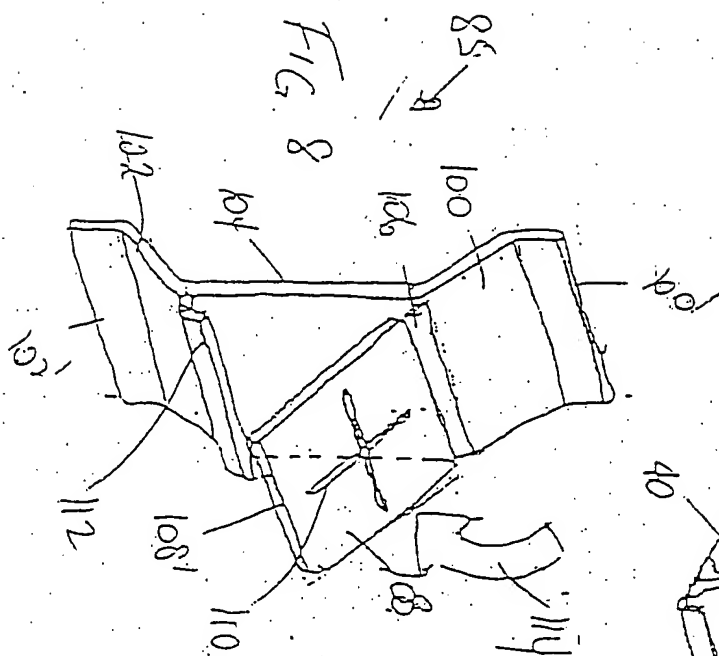


FIG. 8

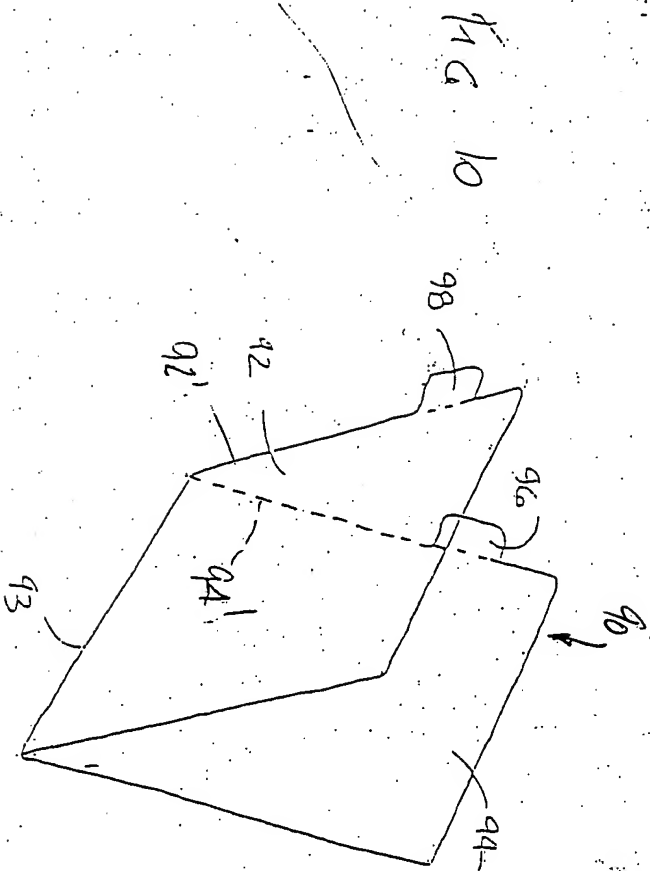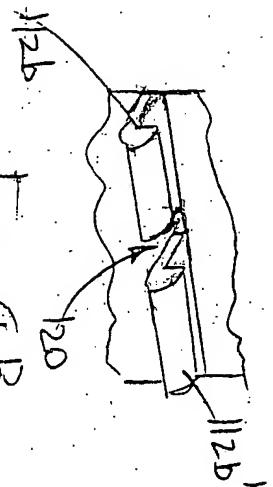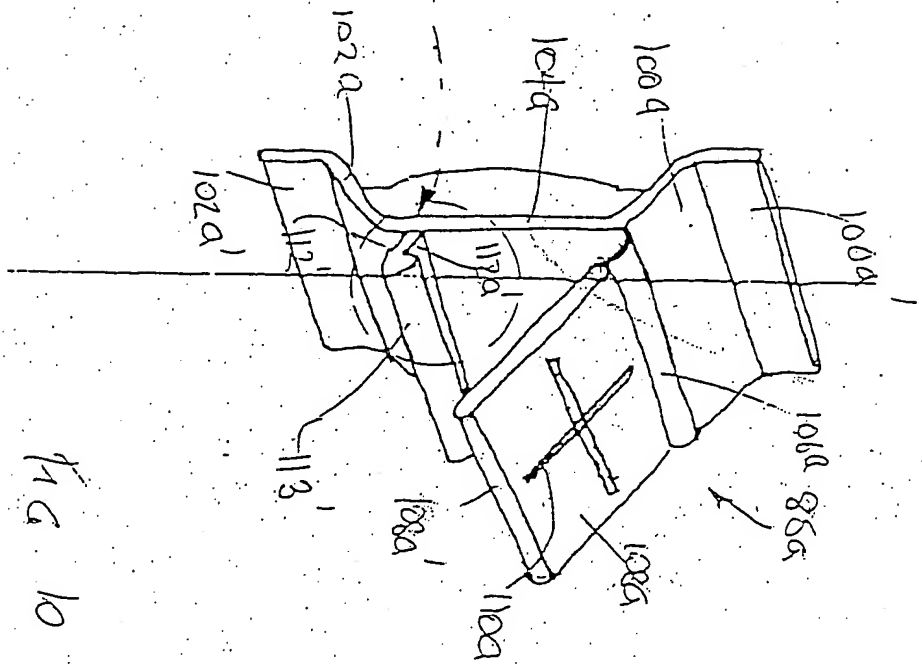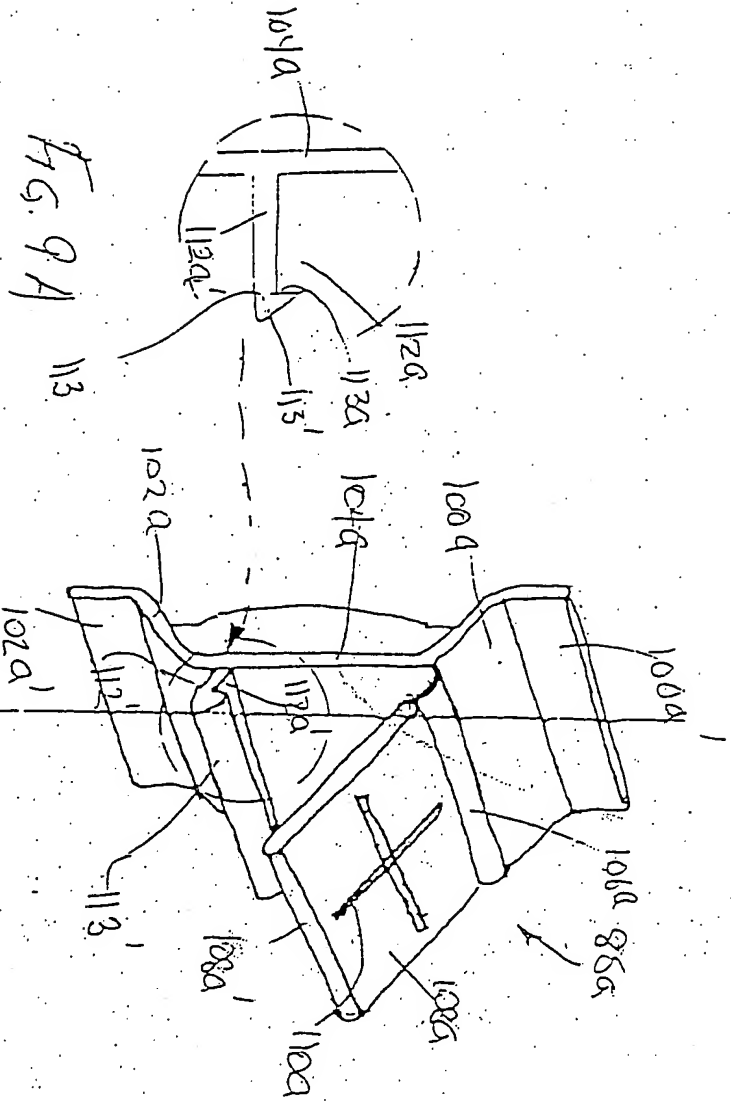

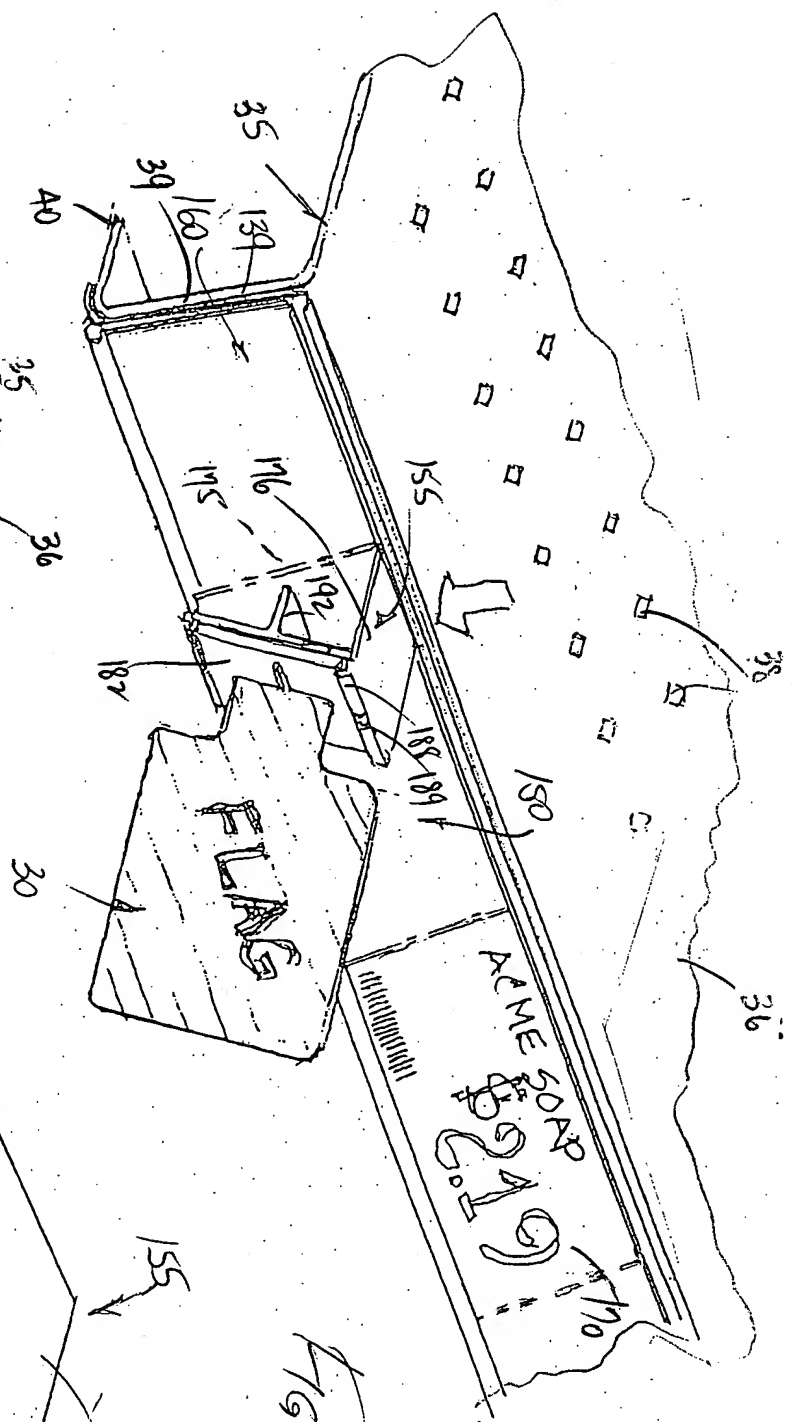

11/15


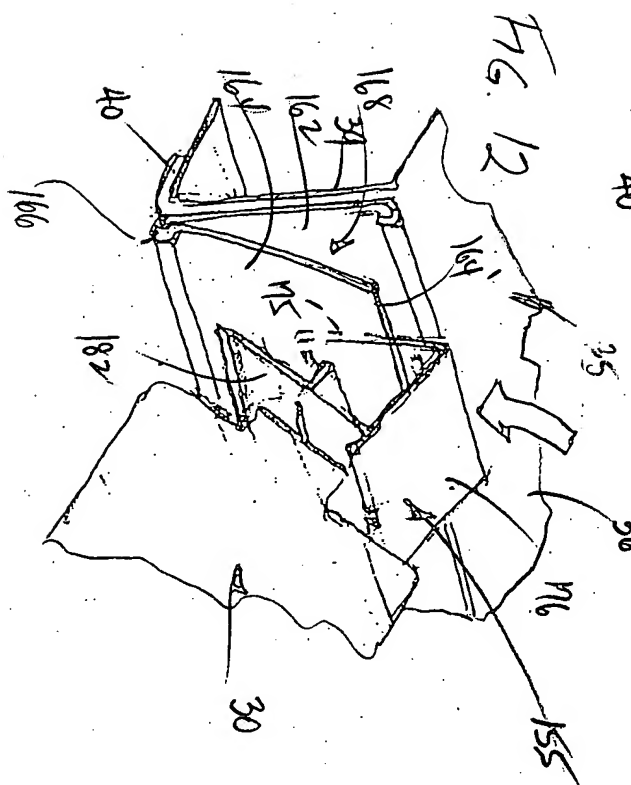


Fig. 12

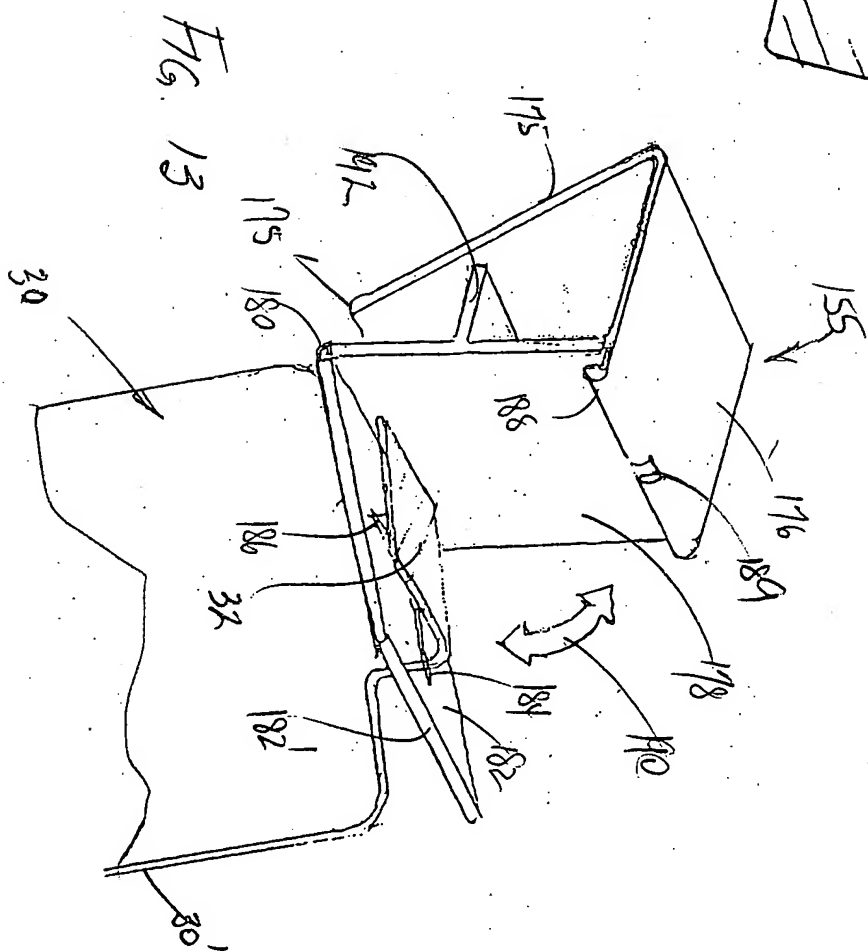

Hg. 13

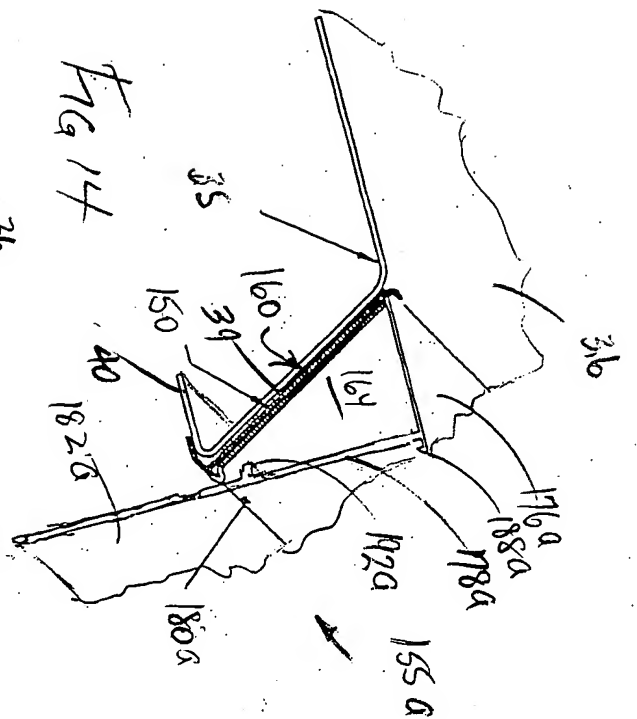


Fig. 14

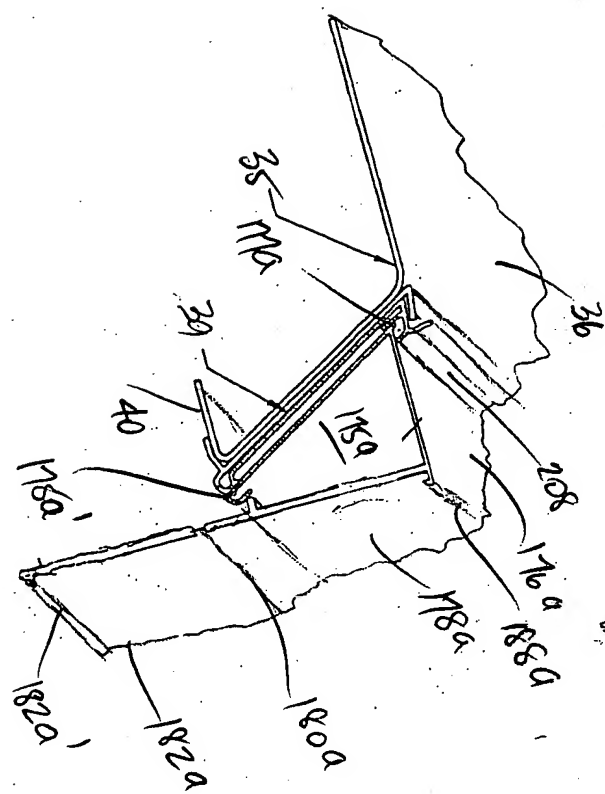


Fig. 18

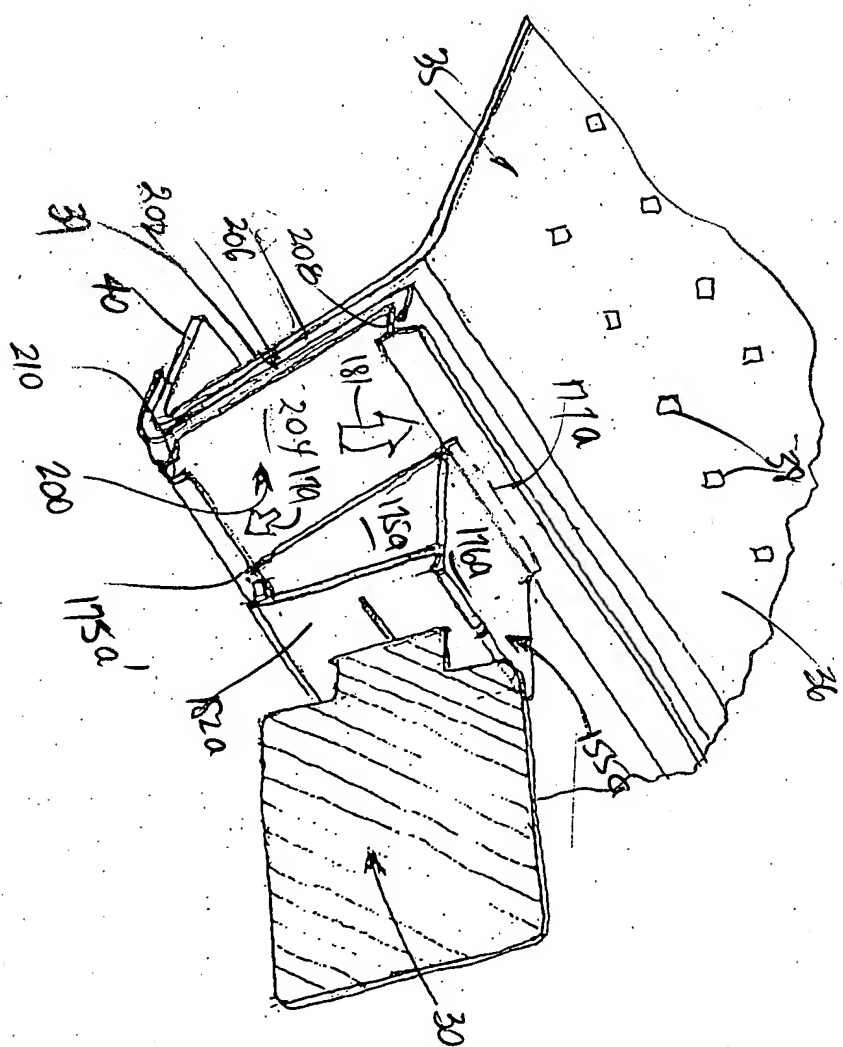


Fig. 17

